

HUMAN CTRP7/C1QTNF7 ELISA KIT

FOR THE QUANTITATIVE DETERMINATION OF
HUMAN CTRP7/C1QTNF7 CONCENTRATIONS
IN SERUM AND PLASMA



ALWAYS REFER TO LOT SPECIFIC PROTOCOL
PROVIDED WITH EACH KIT FOR
INSTRUCTIONS. PROTOCOL MUST BE
READ BEFORE USING THIS PRODUCT.

FOR RESEARCH USE ONLY. NOT FOR USE IN
DIAGNOSTIC PROCEDURES.

PRODUCT INFORMATION:

ELISA NAME	HUMAN CTRP7/C1QTNF7 ELISA
Catalog No.	SK00396-09
Formulation	96 T
Lot No.	
Standard range	1250 - 160,000 pg/ml
Sensitivity	200 pg/ml
Sample Volume	100 µl
Dilution Factor	Optimal dilutions should be determined by each laboratory for each application
Sample Type	Serum, EDTA Plasma
Specificity	Human CTRP7
Calibration	Human CTRP7 recombinant
Intra-assay Precision	4 - 6%
Inter-assay Precision	8 - 10%
Storage	2 – 8° C
This kit contains sufficient materials to run 35 samples duplicated provided that assay is run according to protocol.	

Order Contact:
AVISCERA BIOSCIENCE, INC.
2348 Walsh Ave., Suite C
Santa Clara, CA 95051
USA
Tel: (408) 982 0300
Fax: (408) 982 0301
Email: Sales@AvisceraBioscience.com
Info@AvisceraBioscience.com
www.AvisceraBioscience.com

DESCRIPTION

This CTRP7/C1QTNF7 (H) ELISA Kit contains the necessary components required for the quantitative measurement of recombinant and/or natural human CTRP7 from serum and plasma in a sandwich ELISA format.

This immunoassay contains recombinant human CTRP7 and antibodies raised against this protein. Results from this immunoassay have shown to accurately quantify recombinant and natural CTRP7 samples.

ASSAY OVERVIEW

This assay employs the quantitative sandwich ELISA format. The plate is pre-coated with an antibody specific for human CTRP7. The capture antibody can bind to the human CTRP7 in the standard and samples. After washing the plate of any unbound substances, a biotinylated antibody against human CTRP7 is added to the wells. After another washing of the plate, Streptavidin-HRP Conjugate is added. After the last wash to remove any unbound enzyme, a substrate solution is added to the wells and color develops in direct proportion to the amount of human CTRP7 bound in the standard solutions or samples. A standard curve can be established and sample values can be read off the standard curve.

PROCEDURAL LIMITATIONS

_FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

_This ELISA kit should not be used beyond the expiration date on the kit label.

_Do not mix reagents with those from other lots or sources.

_It is important that the Dilution Buffer selected for the standard curve be consistent with the samples being assayed.

_Each laboratory must determine the optimal dilution factors for the samples being assayed with a pretest. If samples generate values that are not within the dynamic range of the standard curve, further concentrate or dilute the samples as required with Dilution Buffer and repeat the assay.

_Any modifications in buffers, pipetting technique, washing technique, incubation time or temperature, as well as kit age can cause a change in signal.

_Not all interfering factors have been tested in the immunoassay, therefore the possibility of interference cannot be excluded.

COMPONENTS PROVIDED

DESCRIPTION	CODE	QUANTITY
CTRP7 Microplate – 96 well microplate coated with an antibody specific for human CTRP7.	396-09-01	1 plate
CTRP7 Standard – 320 ng/vial of lyophilized recombinant human CTRP7.	396-09-02	1 vial
Detection Antibody Concentrate – 1.2 mL/vial of 10-fold concentrate of lyophilized biotinylated antibody against human CTRP7.	396-09-03	1 vial
Streptavidin-HRP Conjugate – 120 µL/vial of 100-fold concentrated solution of Streptavidin-HRP conjugate.	SAHRP	1 vial
Dilution Buffer – 60 mL of buffered solution with preservative.	DB01	1 bottle
Antibody Diluent Solution – 12 mL of buffered solution with preservative.	DB48	1 bottle
HRP Diluent Solution – 12 mL of buffered solution with preservative.	DB06	1 bottle
Wash Buffer – 50 mL of 10-fold concentrated buffered surfactant with preservative.	WB01	1 bottle
TMB Substrate Solution – 11 mL of substrate solution.	TMB01	1 bottle
Stop Solution – 11 mL of 0.5M HCl.	S-STOP	1 bottle
Plate Sealer	EAPS	1 piece
Plastic Pouch	P01	1 piece

STORAGE

Unopened Kit: Store at 2 – 8° C for up to 8 months. For longer storage, unopened Standard, Positive Control and Detection Antibody Concentrate should be stored at -20° C or -70° C. Do not use kit past expiration date.

Opened / Reconstituted Reagents: Reconstituted Standard (stock) solution and Detection Antibody concentrated solution SHOULD BE STORED at -20° C or -70° C for up to one month. Streptavidin-HRP Conjugate 100-fold concentrated solution and Substrate Solution can be stored at 2 – 8° C for up to 8 months (**DO NOT FREEZE** and **PROTECT FROM**

LIGHT). All other components may be stored at 2 – 8° C for up to 8 months.

Microplate Wells: Return unused strips to the plastic pouch with the desiccant pack. Microplate may be stored for up to 6 months at 2 – 8° C after opening.

ADDITIONAL MATERIALS REQUIRED

- Microplate reader capable of absorbance measurement at 450 nm.
- Microplate shaker (250 – 300 rpm).
- Microplate washer or manifold dispenser.
- 100 mL and 500 mL graduated cylinders.
- Multi-channel Pipette, Pipettes and pipette tips.
- Deionized or distilled water.

PRECAUTION

This kit should be handled by those persons who have been trained in and can follow the principles of good laboratory practice. Wear protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken while handling solutions in this kit to avoid contact with skin or eyes, especially with the stop solution because it contains diluted hydrochloric acid. Wash immediately with water in case of contact on skin or eyes.

SAMPLE COLLECTION AND STORAGE

Serum – Use a serum separator tube (SST). Allow blood to clot for 30 minutes. Centrifuge at 1000 x g for 15 minutes and collect serum. Assay samples immediately or aliquot and store at ≤ -20° C. Avoid repeated freeze-thaw cycles.

Plasma – Collect plasma using EDTA, heparin, or citrate as an anticoagulant. Centrifuge at 1000 x g for 15 minutes and collect plasma. Assay samples immediately or aliquot and store at ≤ -20° C. Avoid repeated freeze-thaw cycles.

Optional: Use Aprotinin (enzyme inhibitor) for ALL sample collection to prevent sample degradation. 0.5 TIU per mL of sample solution.

SAMPLE PREPARATION

Serum and Plasma samples may require dilutions. If the sample concentration assayed exceeds that of the highest standard, a 2- or 4-fold dilution is suggested. A suggested 2-fold dilution is 125 µL sample + 125 µL Dilution Buffer. A suggested 4-fold dilution is 60 µL sample + 180 µL Dilution Buffer.

Optimal dilutions should be determined by each laboratory for each application with a pretest.

Use polypropylene test tubes.


REAGENT PREPARATION

Bring all reagents to room temperature before use.

Wash Buffer – If crystals have formed in the concentrate, warm bottle in a water bath until the crystals have completely dissolved. Dilute 50 mL of Wash Buffer Concentrate into 450 mL distilled or deionized water to make 500 mL of 1x Wash Buffer.

CTRP7 Standard - Reconstitute the CTRP7 standard with 1 mL of **Dilution Buffer (DB01)**. This reconstitution produces a stock solution of 320,000 pg/mL. Allow the standard to sit for a minimum of 15 minutes with gentle agitation prior to making dilutions. Pipette 250 µL of Dilution Buffer into tubes #1 to #8. Use the stock solution to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The **160,000 pg/mL** standard serves as the high standard. The Dilution Buffer serves as the zero standard (0 pg/mL).

TUBE	STANDARD	DILUTION BUFFER	CONCENTRATION
stock	powder	1 mL	320,000 pg/mL
# 1	250µL of stock	250µL	160,000 pg/mL
# 2	250µL of 1	250µL	80,000 pg/mL
# 3	250µL of 2	250µL	40,000 pg/mL
# 4	250µL of 3	250µL	20,000 pg/mL
# 5	250µL of 4	250µL	10,000 pg/mL
# 6	250µL of 5	250µL	5000 pg/mL
# 7	250µL of 6	250µL	2500 pg/mL
# 8	250µL of 7	250µL	1250 pg/mL

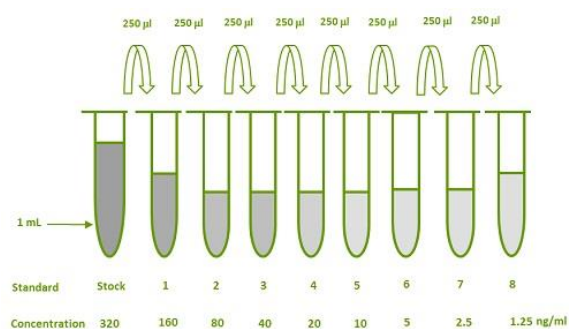

Detection Antibody - Reconstitute the Detection Antibody Concentrate with 1.2 mL of **Antibody Diluent Solution (DB48)** to produce a 10-fold concentrated stock solution. Pipette 10.8 mL of Antibody Diluent Solution into a 15 mL centrifuge

tube and transfer 1.2 mL of 10-fold concentrated stock solution to prepare working solution.

Streptavidin-HRP Conjugate - Pipette 11.88 mL of **HRP Diluent Solution (DB06)** into a 15 mL centrifuge tube and transfer 120 µL of 100-fold concentrated stock solution to prepare working solution. **Note:** 1x working solution of Streptavidin-HRP should be used within a few days (**protect from light**). **DO NOT FREEZE.**

ELISA PROTOCOL

Bring all reagents and samples to room temperature before the start of the assay. Blank, standard dilutions, positive control and samples should be assayed in duplicate. ELISA Protocol may need further optimization.

1. Prepare all reagents and working standards as directed in the previous sections.
2. Remove excess microplate strips from the plate frame, return them to the plastic pouch with the desiccant pack.
3. Add 100 µL of **Dilution Buffer (DB01)** to Blank wells.
4. Add 100 µL of **Standard dilutions from #8-1 or samples** per well. Cover with plate sealer. Incubate for 2 hours on microplate shaker at room temperature.
5. Aspirate each well and wash, repeating the process three times for a total of four washes. Wash by filling each well with **1x Wash Buffer** (300 µL) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
6. Add 100 µL of **Detection Antibody working solution** to each well. Cover with plate sealer. Incubate for 2 hours on microplate shaker at room temperature.
7. Repeat the aspiration/wash as in step 5.
8. Add 100 µL of **Streptavidin-HRP Conjugate working solution** to each well. Incubate for 40 minutes on microplate shaker at room temperature. **Protect from light.**
9. Repeat the aspiration/wash as in step 5.
10. Add 100 µL of **Substrate Solution** to each well. Incubate for 5-10 minutes on microplate shaker at room temperature. **Protect from light.**

11. Add 100 µL of **Stop Solution** to each well. The color in the wells should change from blue to yellow. If the color in the wells is green, or if the color change does not appear uniform, gently tap the plate to ensure thorough mixing.
12. Determine the optical density of each well within 15 minutes, using a microplate reader set to 450 nm.

CALCULATION OF RESULTS

Create a standard curve by plotting the log of the known concentrations of the standard dilutions (x-axis) versus the log of its corresponding O.D. (y-axis) and draw the best fit line through the points. It is recommended to use computer software capable of generating a log-log curve fit to more accurately quantify the standard dilutions.

If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

TYPICAL STANDARD CURVE

This standard curve is provided for demonstration only. A new standard curve should be generated for each set of samples assayed.

STANDARD (PG/ML)	AVERAGE OD450 (CORRECTED)
Blank	0 (0.079)
1250	0.026
2500	0.052
5000	0.112
10000	0.236
20000	0.464
40000	0.732
80000	1.273
160000	2.036

- Lot No.:

SPECIFICITY

Proteins	Cross-reactivity
Human CTRP7	100%
Human CTRP15	0
Human CTRP13	0
Human 12	0
Human CTRP9	0
Human CTRP3	0
Human CTRP2	0
Human Acrp30	0

LINEARITY









To assess the linearity of the assay, pooled research human **serum** samples were diluted with Dilution Buffer (DB01) and assayed.

DILUTION FACTOR	ASSAYED (NG/ML)	FINAL (NG/ML)	RECOVERY (%)
1x	over	over	
2x	28.446	56.892	100
4x	14.890	59.560	105

To assess the linearity of the assay, pooled research human **EDTA plasma** samples were diluted with Dilution Buffer (DB01) and assayed.

DILUTION FACTOR	ASSAYED (NG/ML)	FINAL (NG/ML)	RECOVERY (%)
1x	18.516	18.516	100
2x	10.850	21.700	117
4x	5.379	21.480	116

SUMMARY OF ASSAY PROCEDURE

PREPARE REAGENTS, SAMPLES AND STANDARDS

Add 100 µL of standard dilutions or samples to the well. Incubate 2 hours on the plate shaker at RT.

Aspirate and wash 4 times.

Add 100 µL Detection Antibody working solution to each well. Incubate 2 hours on the plate shaker at RT.

Aspirate and wash 4 times.

Add 100 µL Streptavidin-HRP Conjugate working solution to each well. Incubate 40 min on the plate shaker at RT. Protect from light.

Aspirate and wash 4 times.

Add 100 µL Substrate Solution to each well. Incubate 5-10 min on plate shaker at RT. Protect from light.

Add 100 µL Stop Solution to each well. Read 450nm within 15 min.